

TimeWaver Frequency

A Device for Your Medical Practice



Information for health care professionals

Time**WAVER** 

Notice



The TimeWaver Frequency device is a prescription device intended to be used by healthcare providers in a healthcare setting and is not approved for use in a home environment. The use of the device on a particular patient is solely the decision of the medical professional, who is responsible for having the proper training and exercising his or her informed medical judgment.

In the European Union the TimeWaver Frequency system is a medical device for the treatment of pain in chronic pain, fibromyalgia, skeletal pain and migraine, as well as for the supportive treatment of mental illnesses such as depression, anxiety and related sleep disorders. Always use your TimeWaver Frequency system in accordance with its Instructions for Use

TimeWaver Frequency in Your Medical Practice

The TimeWaver Frequency System is a medical device for the application of microcurrent with the additional benefit of effective novel methods for the promotion of holistic health.

It consists of hardware and software, controlled by a laptop computer, continuously creating the frequencies to be applied and transmitting them to the client by means of various electrodes.



The medical fields of application of the TimeWaver Frequency system are



Symptomatic treatment of chronic pain



Symptomatic treatment of migraine



Supportive treatment of mental illnesses such as depression, anxiety and related sleep disorders

The TimeWaver Frequency system can also be customized; users can develop their own protocols to enhance their applications.



Notice



The analysis and harmonization in the Information Field is not intended to cure, treat, mitigate, diagnose or prevent any disease or medical condition. It is intended to give the professional user the option, in a holistic context, to derive helpful information from findings from the Information Field. Each professional user should evaluate, based on their own experience, whether the application is useful in their practice.

The Individualized Microcurrent Frequency (IMF) and Frequency Specific Microcurrent (FSM) programs of the TimeWaver Frequency system are not intended to cure, treat, mitigate, diagnose, or prevent any disease or medical condition. The terms used in the programs, databases and modules do not constitute statements concerning their effects. Information from the TimeWaver system should always be critically questioned and, if necessary, verified with further procedures. The TimeWaver Frequency system should always be used within the scope of the user's professional practice, license or certification and in accordance with the Instructions for Use and company-provided manual. The use of the TimeWaver Frequency system should not be treated as a substitute for a physician's advice, diagnosis or choice of therapy. The responsibility for the correct diagnosis and therapy always lies with the medical professional. The purpose of the product is to provide the professional user with a tool to explore application options.

Frequency Application for Holistic Health

Marcus Schmiede had already been successfully working with Information Field technology* and application in various disciplines for several years when Portuguese researcher Nuno Nina suggested to him combining Information Field technology with the application of microcurrent.



Nuno Nina



Marcus Schmiede




* Information Field technology is a proprietary technology of TimeWaver. It is based on the theory that the Information Field is the non-material area through which spirit and matter communicate. It reflects what we consider to be the spiritual meaning of life events. The existence of such a field is discussed in scientific literature.

Analysis in the Information Field is designed to search for the information patterns that contribute to the harmonization of the Information Field. For this purpose, a priority is assigned to contents such as descriptive sentences, arranged in lists, by evaluating the data of a physical noise generator. In our users' experience, this priority reflects the relevance for the user. An analysis in the Information Field reflects a combination of factors at the time the analysis is done, including the intention of the user. An analysis at a different time may have a different result due to changes in the environmental variables.

TimeWaver has conducted unblinded before/after surveys in controlled and randomized groups of participants. These surveys suggest that the participants' wellbeing was higher after the application. We attribute this to the harmonization of the Information Field, in which the life energy, also called chi (or qi) and prana, is brought back into flow. This has not been confirmed by independent studies

Frequencies and Harmony

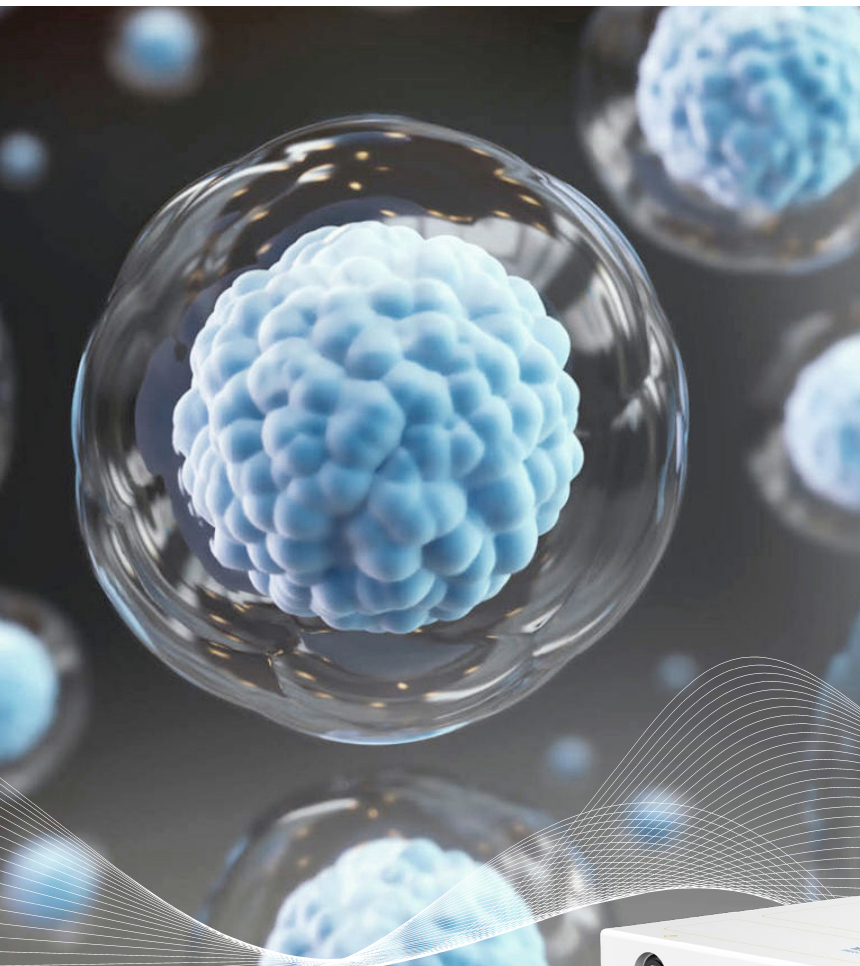

Frequencies Speak the Language of the Body

We only understand maybe one percent of this rich language today, but with just this one percent we can achieve very good results and promote wellbeing in many different ways.



Harmonizing the Bioenergetic Field

The applications for holistic health of the TimeWaver Frequency system are designed to harmonize imbalances in the Bioenergetic Field. We believe these imbalances are mostly invisible influences that can affect people in all areas of life and often have emotional or stress-related causes.

The TimeWaver Frequency system is designed to analyze frequencies in the Information Field and then apply the thusly identified Individualized Microcurrent Frequencies (IMF*).



Unique Information Field Technology

The TimeWaver Frequency system combines TimeWaver Information Field application with Individualized Microcurrent Frequency (IMF) programs, based on the developments and experience of Nuno Nina, a Portuguese researcher and clinical director. The system includes modules to analyze the most suitable frequencies from more than 50,000 Gold Frequencies.

There is a wide range of applications, from wellbeing and vitality to sports and stress management.

*"Individualized Microcurrent Frequencies" ("IMF") is a proprietary technology of TimeWaver. It uses the data from a physical noise generator to assign a priority to frequencies that professional users' experience indicates have the highest relevance for the user. The Individualized Microcurrent Frequency (IMF) programs are designed to support wellbeing through the harmonization of the Bioenergetic Field.



Frequency Application: Support for Your Practice

The application is non-invasive; the clients do not feel more than a slight tingling during this procedure. During the application, which lasts approximately 20-60 minutes, the clients can relax, let the frequencies take effect and recover from everyday life.

Through the intelligent functions of TimeWaver technology, the entire workflow can be automated and compiled in individual client-specific protocols. The system independently processes the various frequency sequences using its automation functions. You only need to check the status and progress of the application from time to time.

With the TimeWaver Frequency system working independently, requiring only minimal operator intervention, its users have more time to attend to other clients. This is confirmed by the experience of thousands of users worldwide.



What TimeWaver Frequency Can Do for You



A clear and easily understood application protocol



Detailed training courses at the TimeWaver Academy



Easy to reproduce procedures



Time saving automation



An easy to delegate method



Worldwide application since 2010



More than 50 million applications of Individualized Microcurrent Frequency (IMF) programs



The Cell as a Mirror of the Body

A Strong Cell as the Basis for Wellbeing

Cell researchers Dr. Robert O. Becker and Dr. Bjorn Nordenstrom, the latter being a former chairman of the Nobel Assembly, discovered that a decrease in cell membrane tension is often associated with a decline in health.

But why does cell membrane voltage decrease in the first place? According to this model, an acidic cellular milieu is the major cause, meaning that there are too few electrons surrounding the cell, causing the pH value to drop. This is where TimeWaver Frequency comes in: Its goal is to harmonize the Bioenergetic Field of the cell.



Increased
amino acid
transport

Up to
40%

Increased
protein
synthesis

Up to
70%

Increased
ATP
production

Up to
500%

Note: Clinical Orthopaedics and Related Research No. 171, November-December 1982. This animal study refers to the effects of microcurrent and does not pertain to the TimeWaver Frequency system itself, but to the basic mechanisms on which it builds. These results have not been confirmed by other studies so far and the transfer of the results to the TimeWaver Frequency system would be speculative.

Individualized Microcurrent Frequencies (IMF)



Determining Frequencies in Real Time

The Individualized Microcurrent Frequency (IMF) application of the TimeWaver Frequency system is very innovative: The system permanently determines the frequencies to be applied in real time and continuously adapts them to the client during application.

Using the resonance analysis function, the system analyzes the duration of the respective frequency matched to the client and checks the progress of the applied frequencies. At the appropriate point in time, the system automatically switches to the next frequency and applies it until it is no longer needed.



The Information Field Module: Analyzing Deep Backgrounds

The Information Field Module of the TimeWaver Frequency system is designed to analyze backgrounds and potential interconnections in the Information Field on an emotional and systemic level. In our experience, this is a good preparation for the frequency application and an elementary part of the TimeWaver Frequency system. It helps you in analyzing which frequencies are suggested for a specific application and to draw conclusions about possible correlations found in the Information Field. This should enable you to harmonize the Bioenergetic Field of your clients by applying those frequencies.

The Information Field layer of the TimeWaver Frequency system contains an extensive database on different levels in the Bioenergetic Field, pertaining to a number of topics.*

In addition, the TimeWaver Frequency system analyzes, within the Information Field, which positive information could be useful, and sends this information into the Information Field.

*The content of the TimeWaver Frequency databases is based on the practical experience of the experts who created them. They have not been confirmed by independent studies.

TimeWaver Frequency McMakin

Frequency Specific Microcurrent (FSM*) for Vitality and Wellbeing



The TimeWaver Frequency McMakin system is based on over 25 years of experience by chiropractor **Carolyn McMakin** with dual-channel applications of Frequency Specific Microcurrent (FSM). More

than 120 automatic FSM application protocols are available for a variety of applications and disciplines; these can easily be expanded to include additional customized protocols.

FSM applies only minimal current levels which are below the threshold of perception for the human organism. Individualized Microcurrent Frequency (IMF) applications and Frequency Specific Microcurrent (FSM) can be combined to benefit from both methods.


The TimeWaver Frequency McMakin system is both a device and a method. Carolyn McMakin, D.C. is renowned worldwide as a pioneer of dual frequency application, especially in the field of competitive sports and imbalances in the Bioenergetic Field.

The most important protocols of her method, in use for over 20 years, have been adapted to the TimeWaver Frequency system and the result is the TimeWaver Frequency McMakin system. Each of these protocols contains specific frequency pairs that always possess the same structure: The first frequency is related to the purpose, for example vitalization. The second frequency defines the target, for example the Bioenergetic Field of a joint.


*“Frequency Specific Microcurrent” (“FSM”) is a proprietary mode of action used by TimeWaver. It uses two outputs in parallel to transmit frequency modulated microcurrent to the client via electrodes. The frequency pairs, duration, frequency, intensity and naming of the programs are based on the practical experience of the experts who created them. The frequency programs are designed to support wellbeing through the harmonization of the Bioenergetic Field. TimeWaver has conducted unblinded before/after surveys in controlled and randomized groups of participants. These surveys suggest that the participants’ wellbeing was higher after the application. We attribute this to the harmonization of the Bioenergetic Field, which we refer to as the energy flow of life, traditionally also called chi (or qi) and prana. This has not been confirmed by independent studies.

TimeWaver Frequency vs. TimeWaver Frequency McMakin

TimeWaver Frequency, being a multi-purpose system, has a broad range of applications, whereas TimeWaver Frequency McMakin specializes in harmonizing the Bioenergetic Field of joints and bones by using FSM (Frequency Specific Microcurrent). Both applications (Individualized Microcurrent Frequencies and Frequency Specific Microcurrent) can be operated on the same TimeWaver Frequency hardware device.

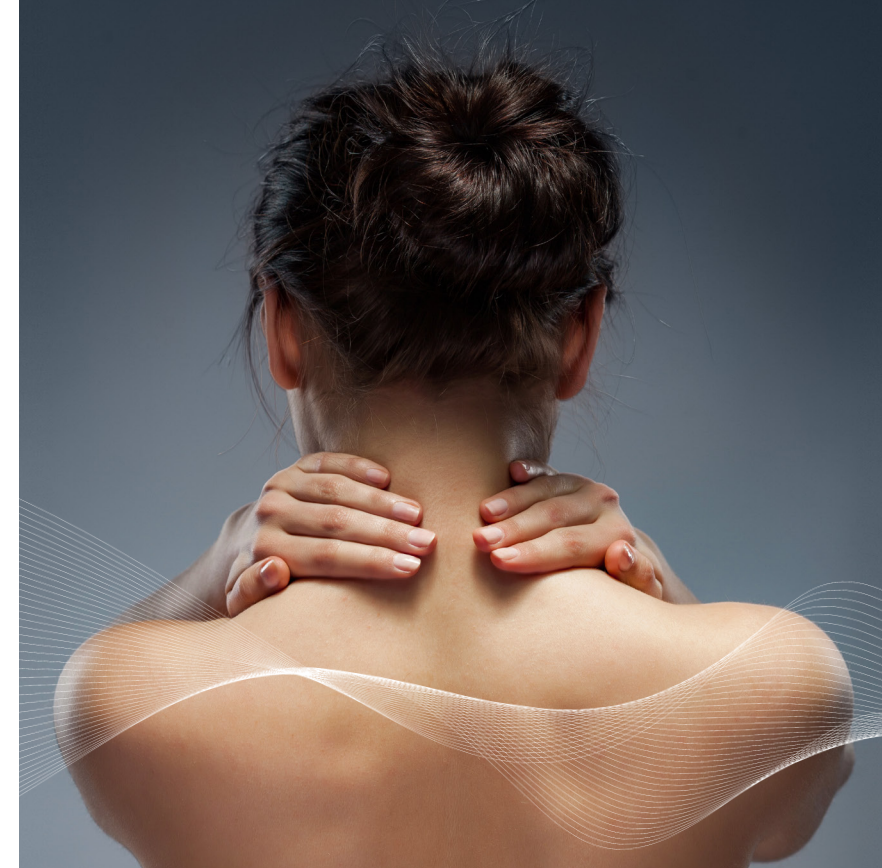

Experience the World of TimeWaver

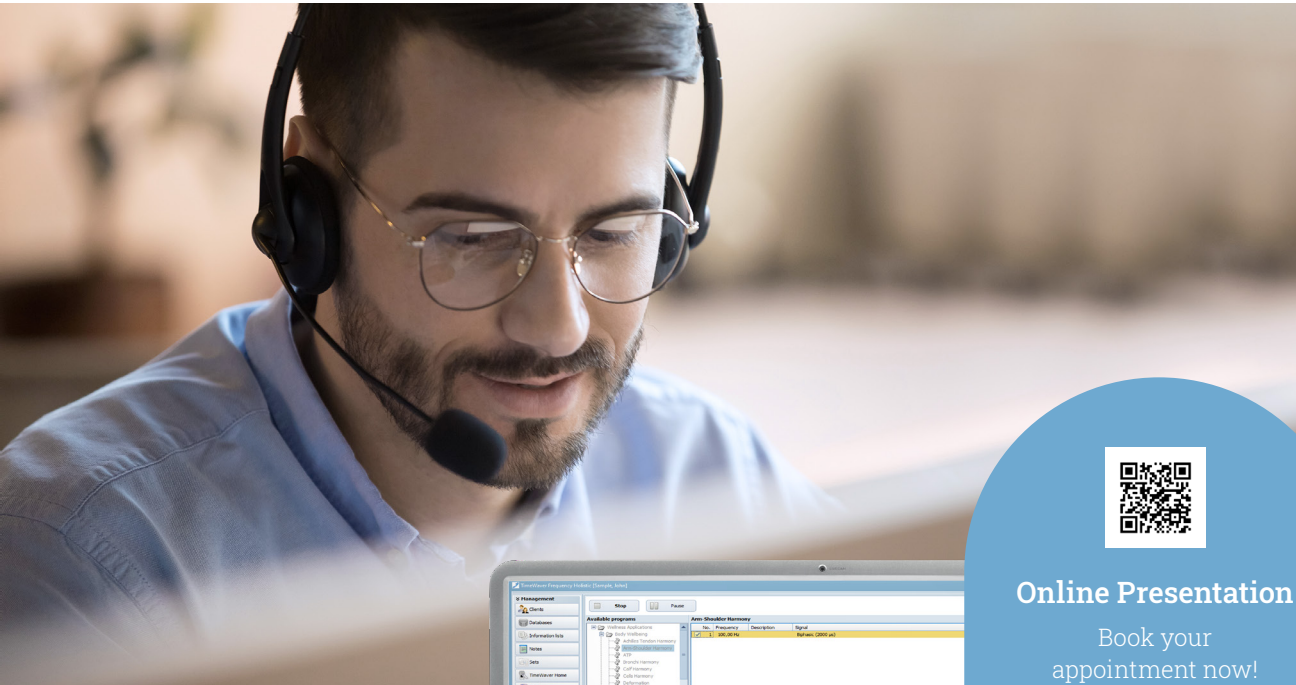

Online Presentation

Book your
appointment now!



Seeing Means Understanding

TimeWaver Information Field technology can be understood by interested individuals and new users primarily through their own experience.

A personal online presentation by an expert user representative will let you understand the TimeWaver systems, learn some interesting facts about their benefits for relationships, career, wellbeing etc. and maybe even experience the potential of their wide range of applications in your life and your business.

In short: the perfect way to enrich your life and/or start your future work with TimeWaver!



© 2022 TimeWaver Home GmbH

All rights reserved. Any publication - especially on the internet -, electronic copying and reprint, also partially, is prohibited. Exceptions only with prior written approval by TimeWaver Home GmbH.

Disclaimer: Science does not acknowledge the existence of the Information Field, its analysis, harmonization and other importance due to the lack of scientific evidence. Individualized Microcurrent Frequency (IMF) and Frequency Specific Microcurrent (FSM) programs are not acknowledged by conventional medicine due to the lack of scientific evidence in the sense of conventional medicine. Use of TimeWaver products, programs or information is at the user's own risk and subject to the user's discretion and professional judgment. The TimeWaver companies specifically disclaim responsibility for user decisions related to the use of TimeWaver products or services that are outside the scope of the Instructions for Use and company-provided manual.

2022-12-12



TimeWaver Home GmbH

Schloss Kränzlin · Darritzer Str. 6
16818 Kränzlin · Germany
Tel. +49 3391 40022 - 11

info@timewaver.com
www.timewaver.com

TimeWAVER 